


Cadenza HS-C18

150 x 3 mm

HPLC COLUMN APPLICATION

Minoxidil and Metabolite in Bovine Serum

血清中のミノキシジルと代謝物

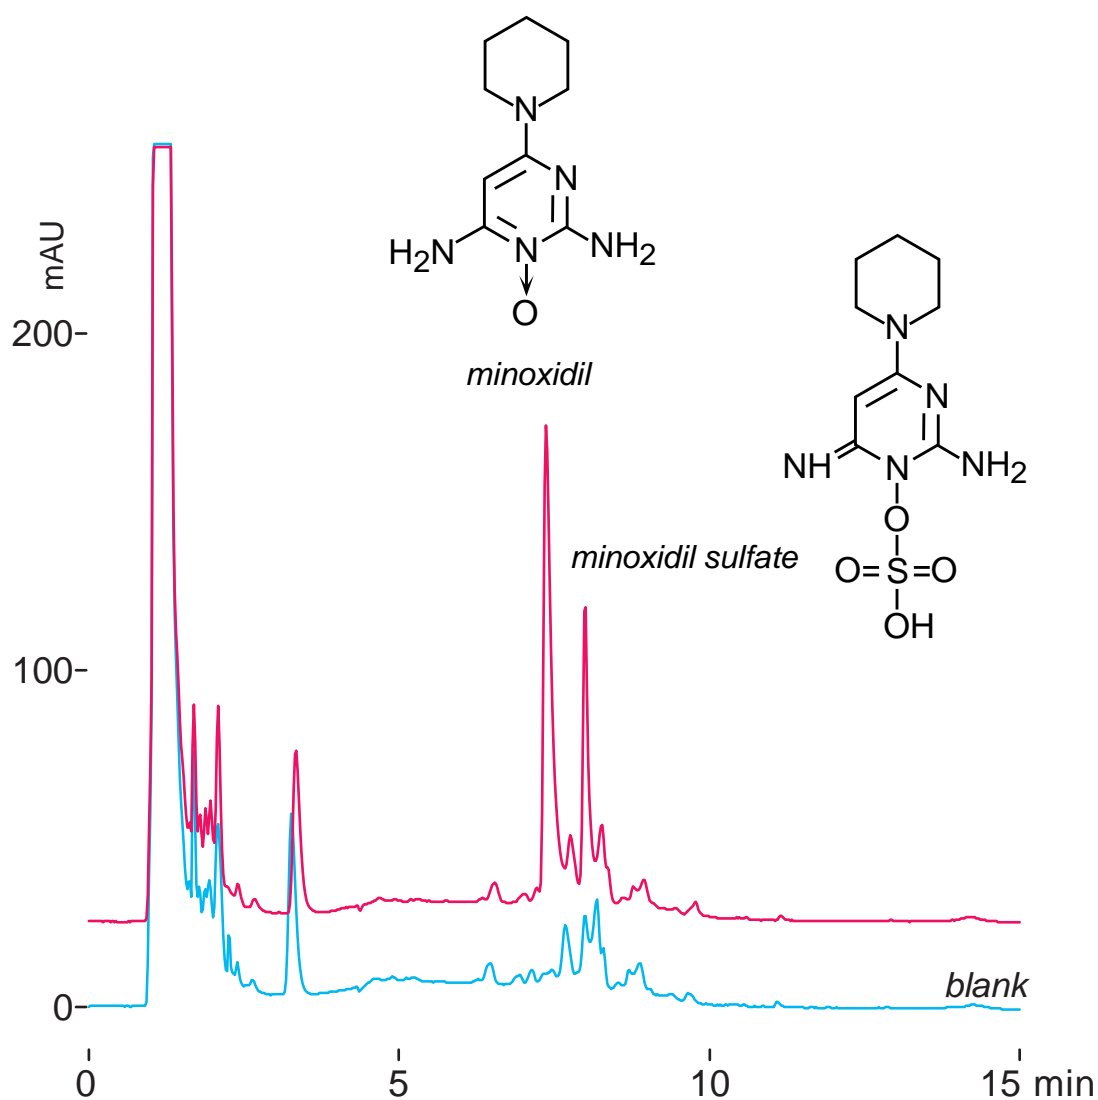

Cadenza HS-C18, 150 x 3 mm

A: 50mM ammonium acetate

B: acetonitrile

0-70%B (0-14min)

0.4 mL/min, 37 °C, 260 nm, 20µL (100-300ng)