



Presto FF-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

glycogen

グリコーゲン (牡蠣由来)

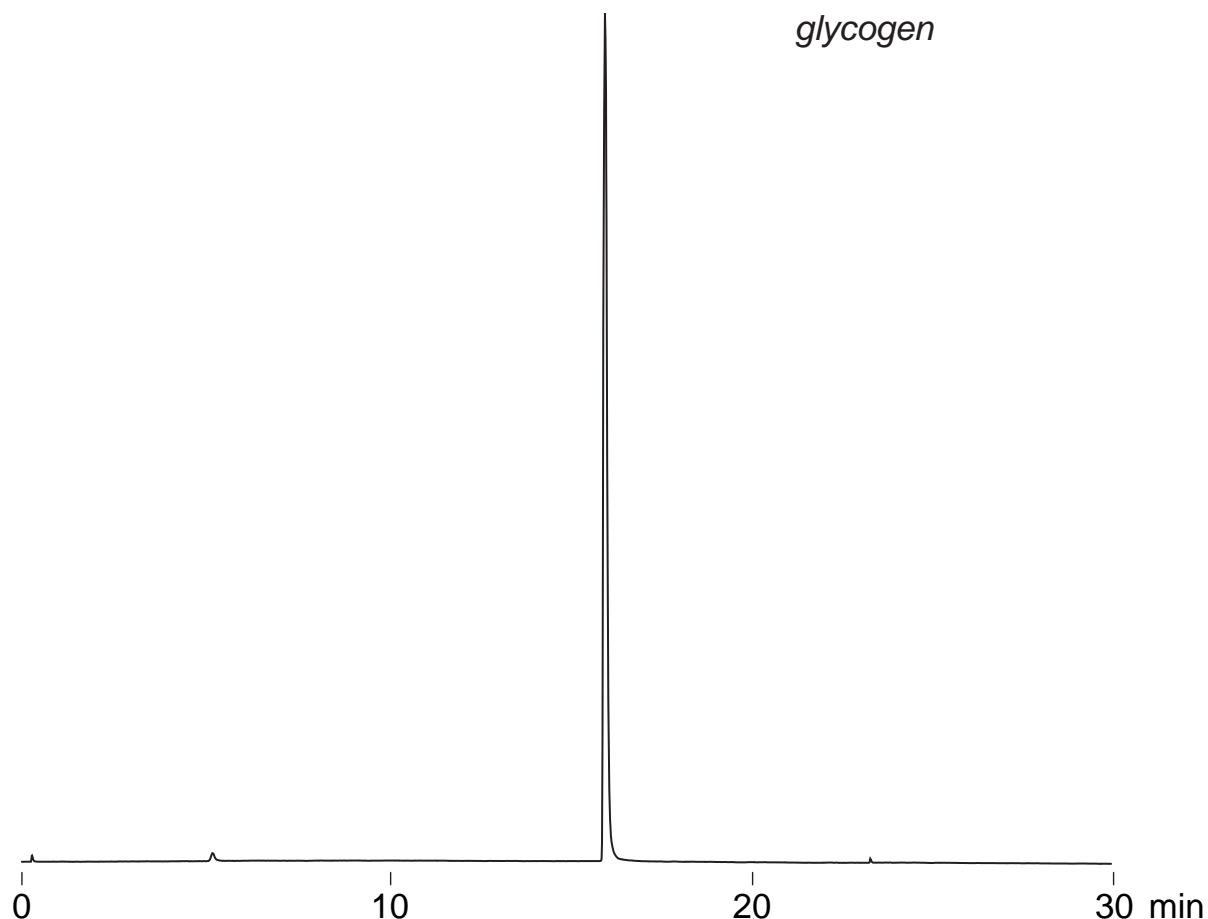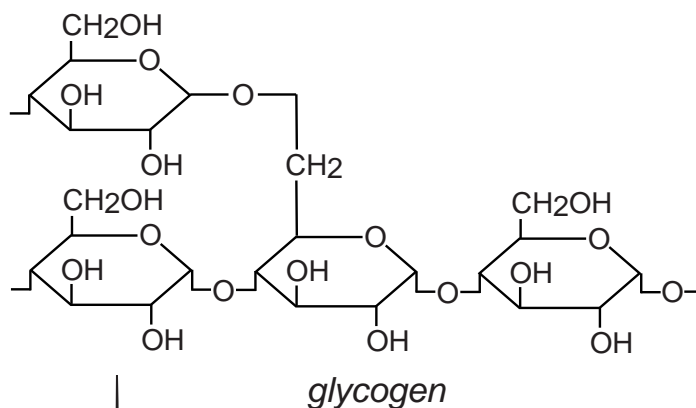

Presto FF-C18, 250 x 4.6 mm
 A: water / formic acid = 100 / 0.1
 B: acetonitrile / formic acid = 100 / 0.1
 0-75%B (0-30min)
 0.3mL/min (15MPa), 37°C
 ELSD (spray chamber 50°C, drift chamber 100°C)
 10µL (2mg/mL, water)