
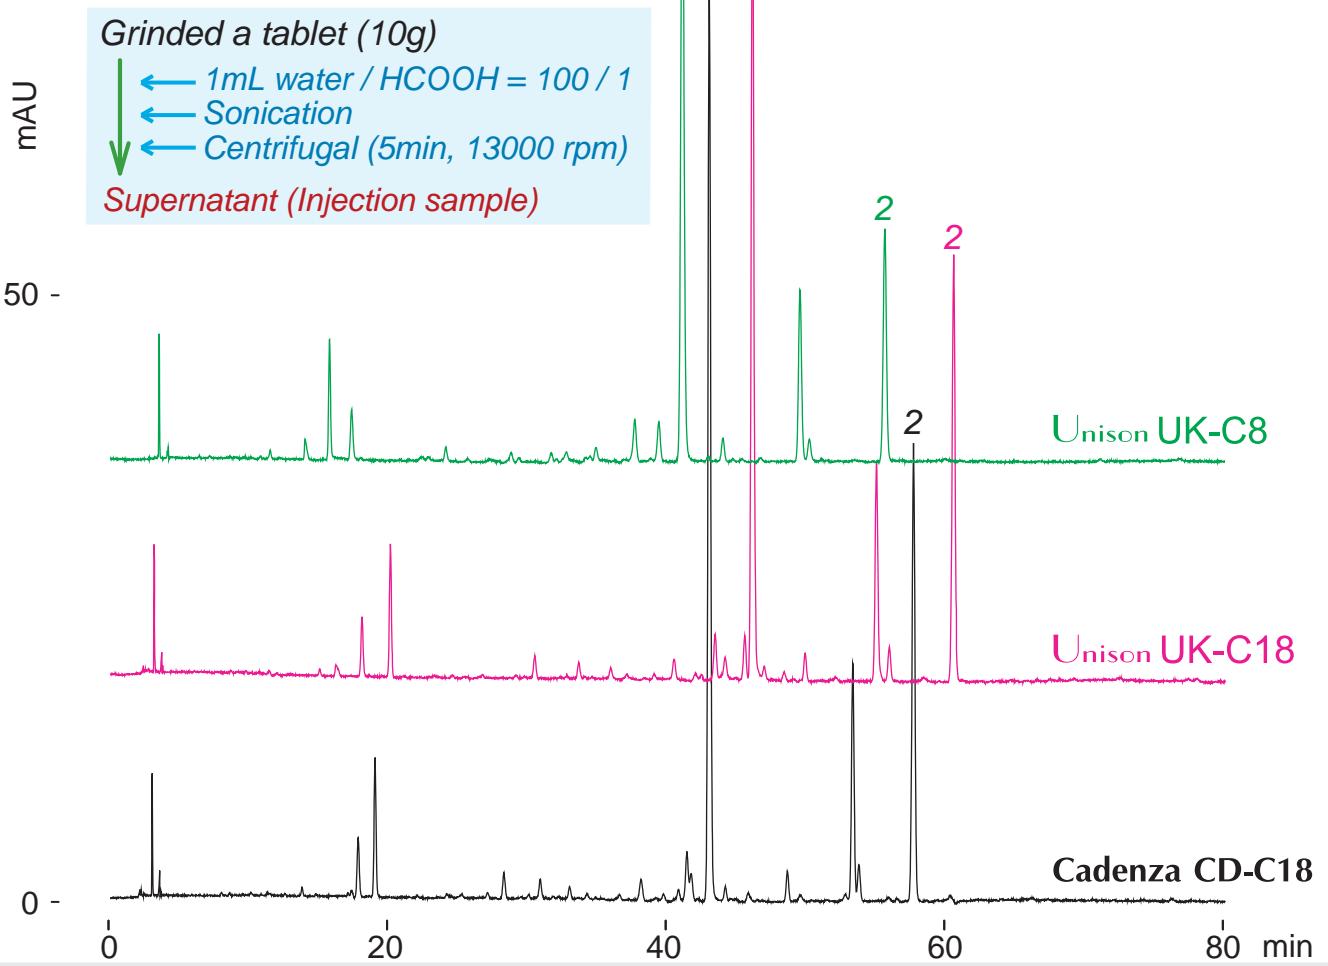
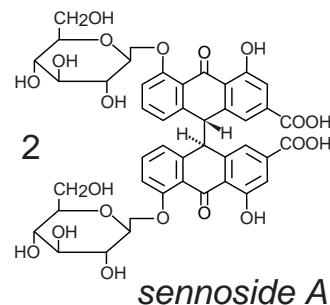


250 x 4.6 mm

HPLC COLUMN APPLICATION

Sennoside (Laxative)

センノシド(緩下剤)

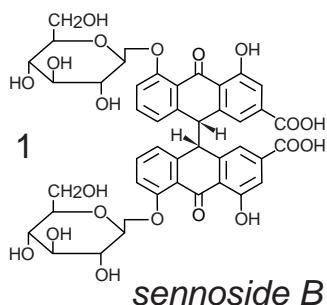

250 x 4.6 mm

A: water / acetonitrile / formic acid = 90 / 10 / 0.1

B: water / acetonitrile / formic acid = 50 / 50 / 0.1

0% B (0-1min), 0-30% B (1-80min)

1.0mL/min (18MPa), 37°C, 370nm

10µL (0.6mg/mL, water / formic acid = 100 / 1)