


Presto FF-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

Sorbitan fatty acid ester

ソルビタン脂肪酸エステル

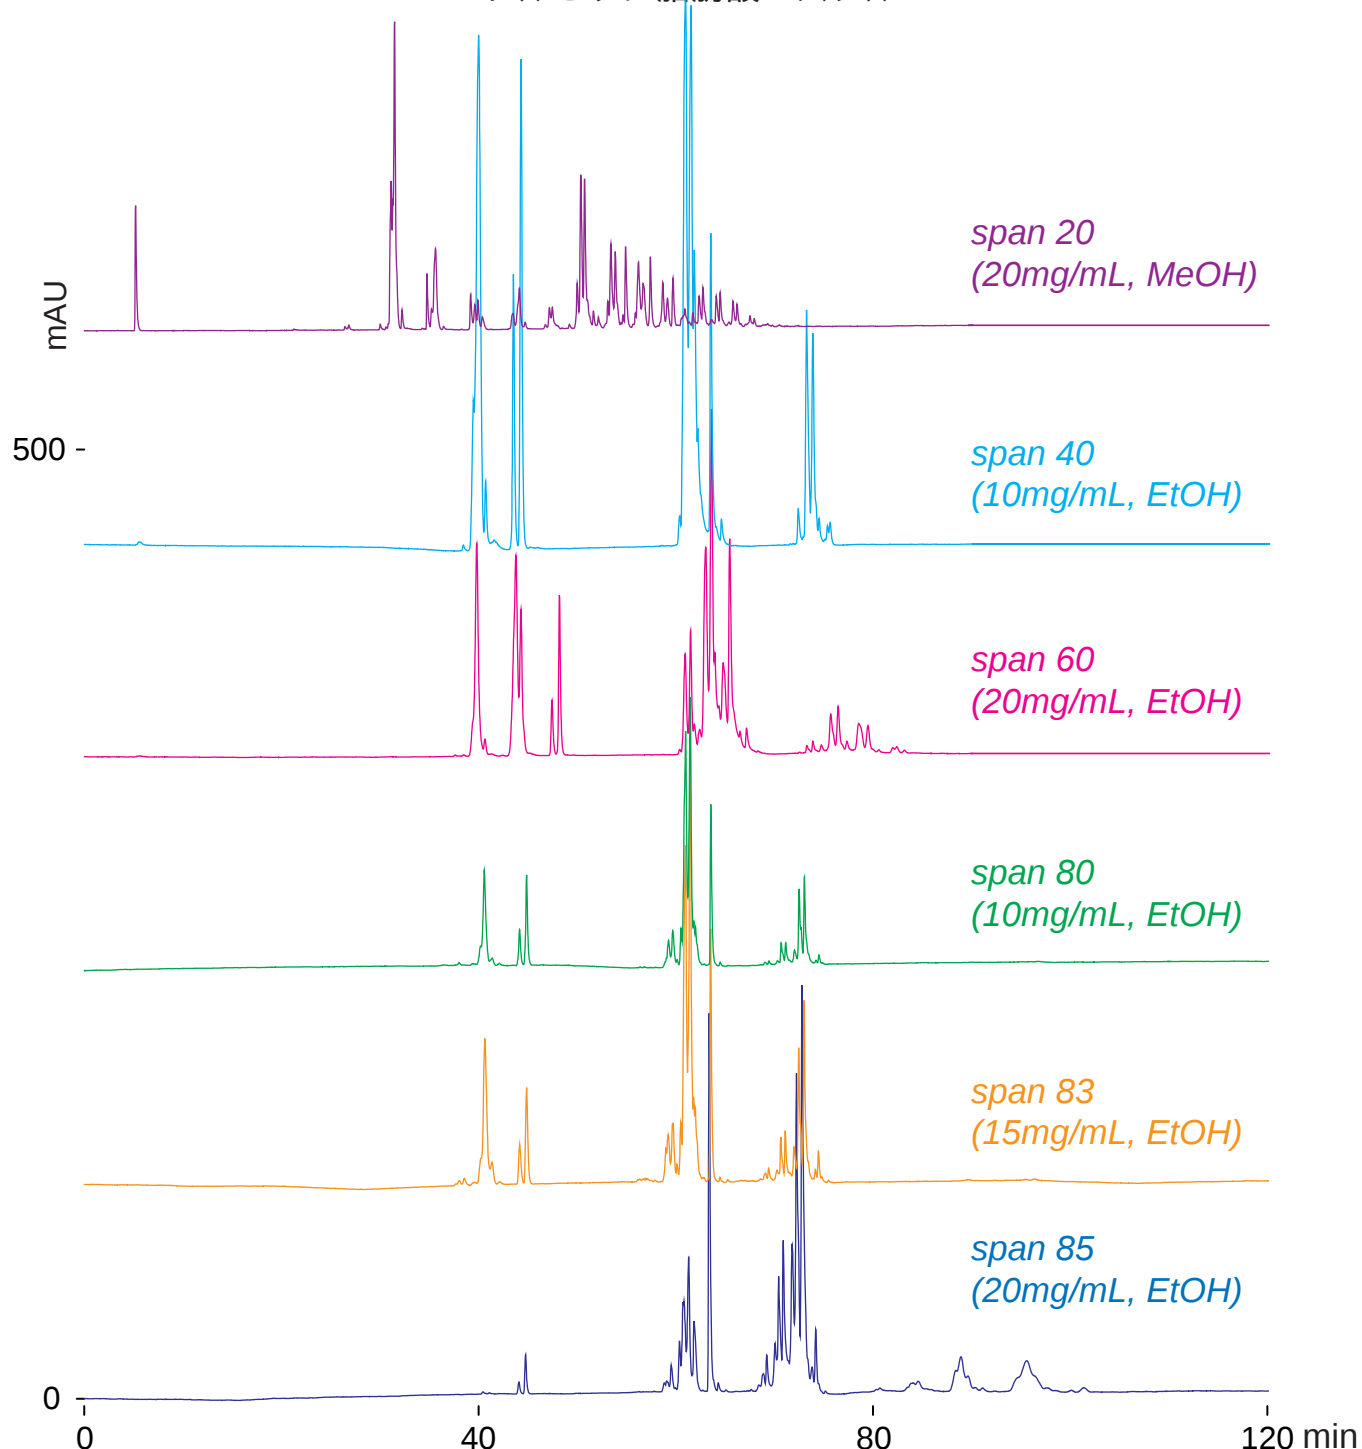

A: water / acetic acid = 100 / 0.1, B: acetonitrile / acetic acid = 100 / 0.1
 0-100%B (0-60min), 100%B (60-120min)
 0.3mL/min (24MPa), 37°C, 10 μ L
 ELSD (spray chamber 70°C, drift chamber 100°C)