








Unison UK-C18

100 x 3 mm

HPLC COLUMN APPLICATION

LC-MS: Hindered amine light stabilizers

ヒンダードアミン光安定剤の LC-MS 分析

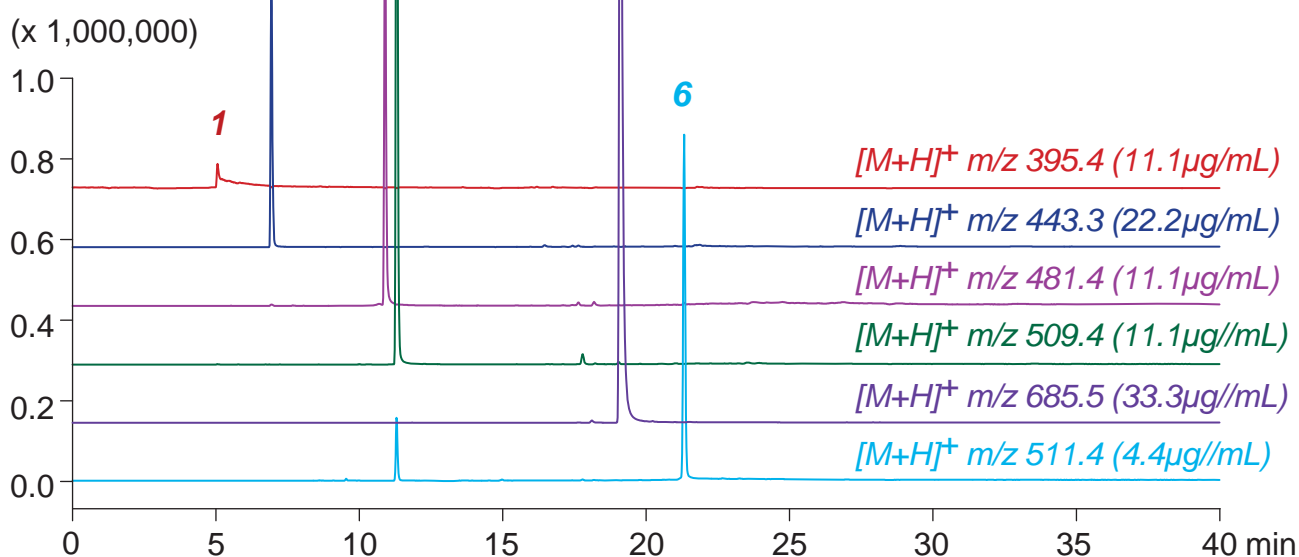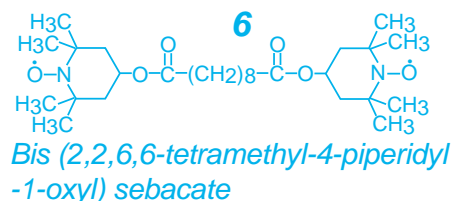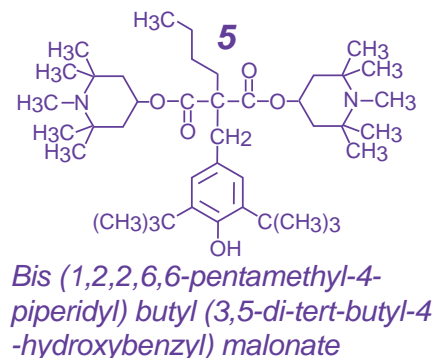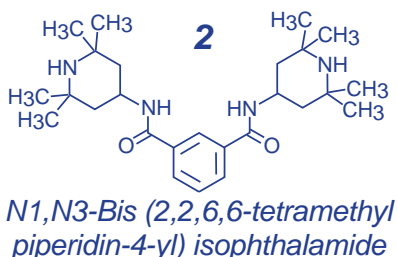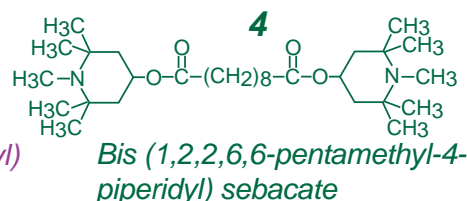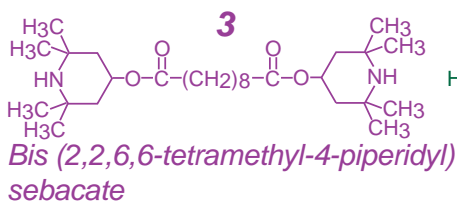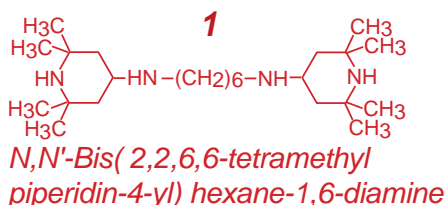

Unison UK-C18, 100 x 3 mm  
 A: 100mM ammonium formate  
 B: 100 mM ammonium formate / acetonitrile = 10 / 90  
 0%B (0-1min), 0-100%B (1-20min), 100%B (20-40min)  
 0.4mL/min (7MPa), 37°C, Single Quad. MS (ESI)  
 1μL (4.4-33.3μg/mL, DMF / 100mM HCOONH<sub>4</sub> = 70 / 30)