

Nardis ND-NX MF


Nardis ND-NX

150 x 2 mm


HPLC COLUMN APPLICATION

Adenosine phosphates


アデノシンリン酸の分析

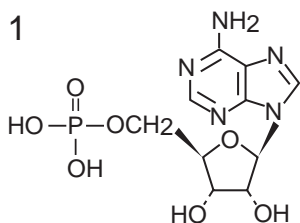


AMP (0.2mg/mL)

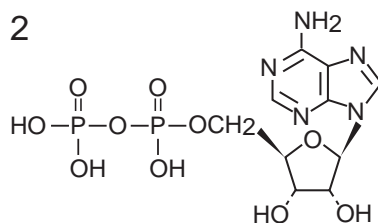

ADP (0.2mg/mL)

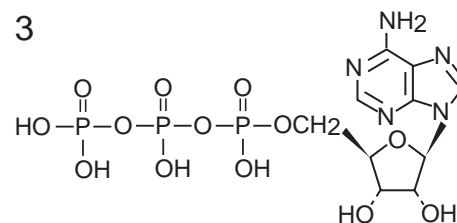

ATP (0.2mg/mL)

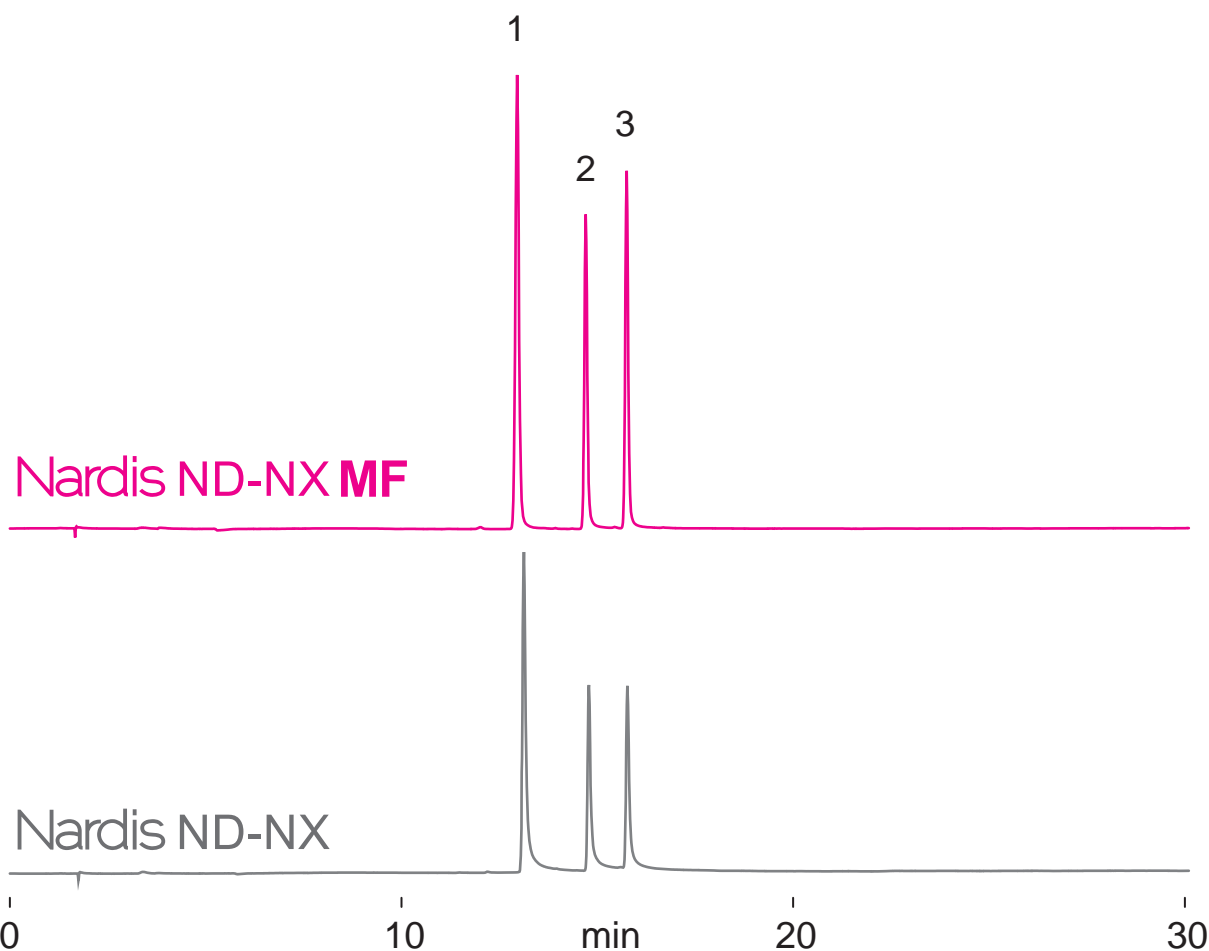

150 x 2 mm

A: acetonitrile

B: acetonitrile / 100mM ammonium acetate = 10 / 90

20-90%B (0-30min)

0.2mL/min (5MPa), 37°C, 260nm

2.0µL (200µg/mL, 100mM ammonium acetate)