

Unison UK-Amino


Nardis ND-NX

150 x 4.6 mm

HPLC COLUMN APPLICATION

Fosfomycin

ホスホマイシンの分析

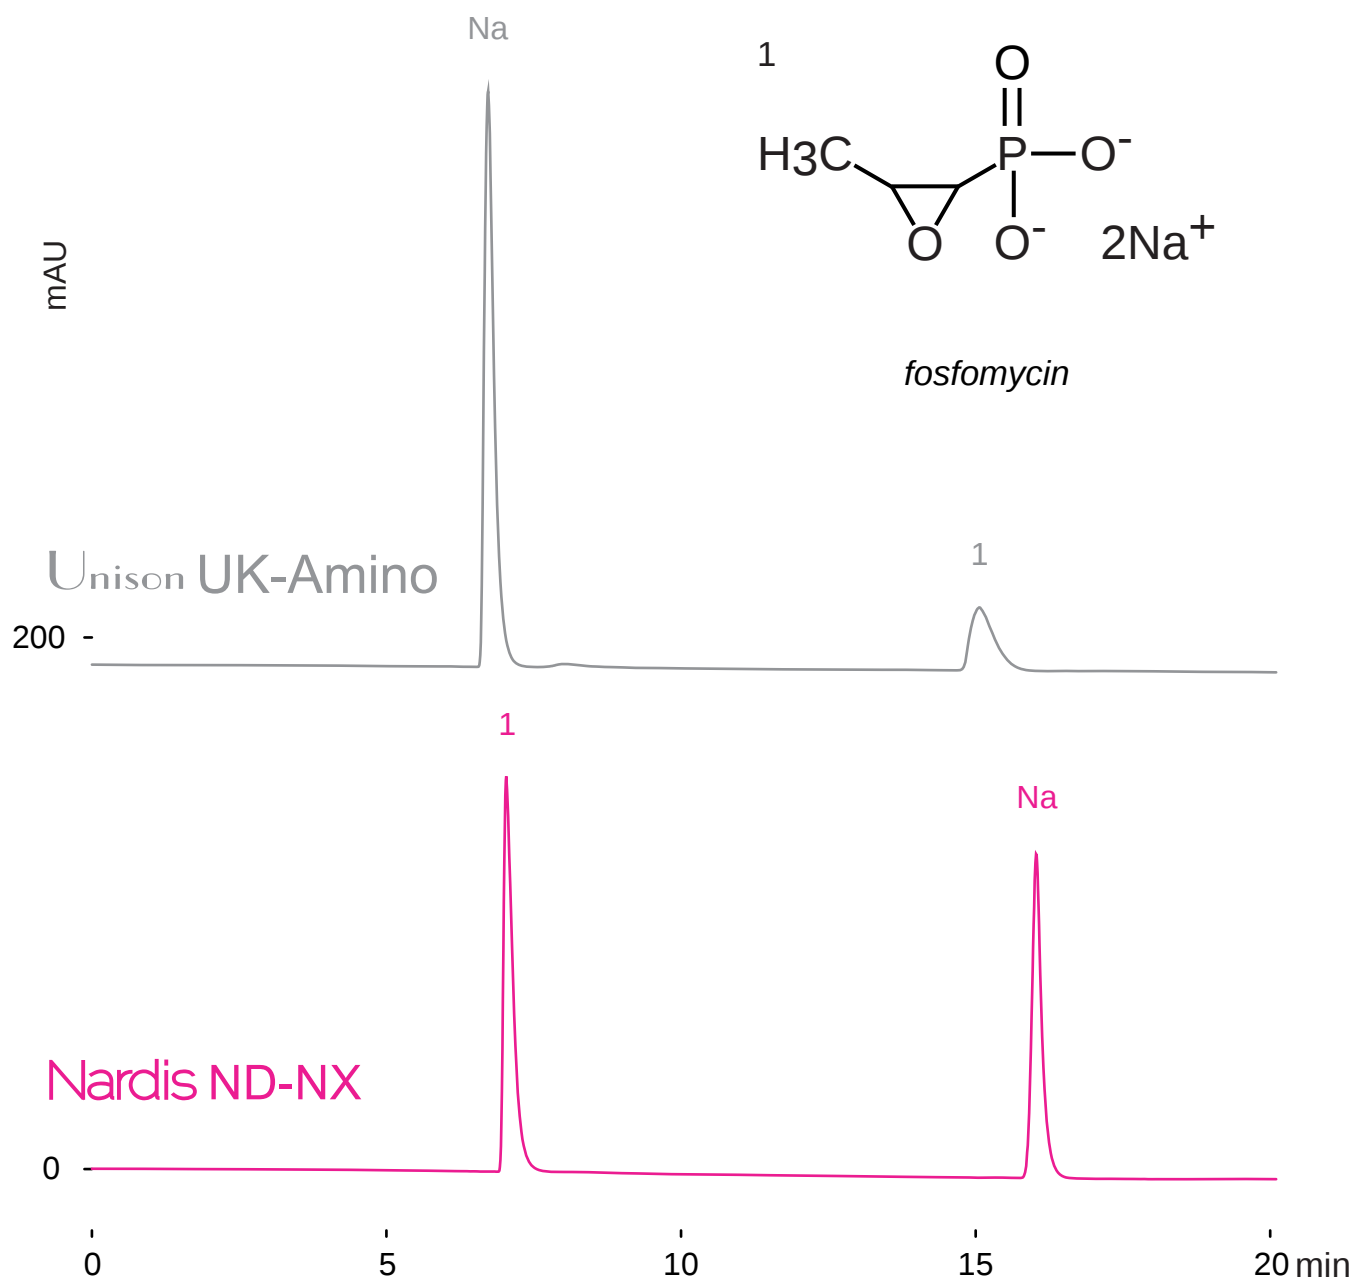

150 x 4.6 mm

A: acetonitrile

B: 100mM ammonium acetate

0 -100%B (0 -15 min), 100%B (15 -20 min)

1.0 mL/min (6 -7 MPa), 37°C

ELSD (spray chamber 70°C, drift chamber 70°C)

10 µL (5mg/mL, water)