


Nardis ND-NX  
Unison UK-Amino  
Unison UK-Silica

150 x 4.6 mm

HPLC COLUMN APPLICATION

Guanidine hydrochloride (protein denaturant)

グアニジン塩酸塩 (タンパク質変性剤)

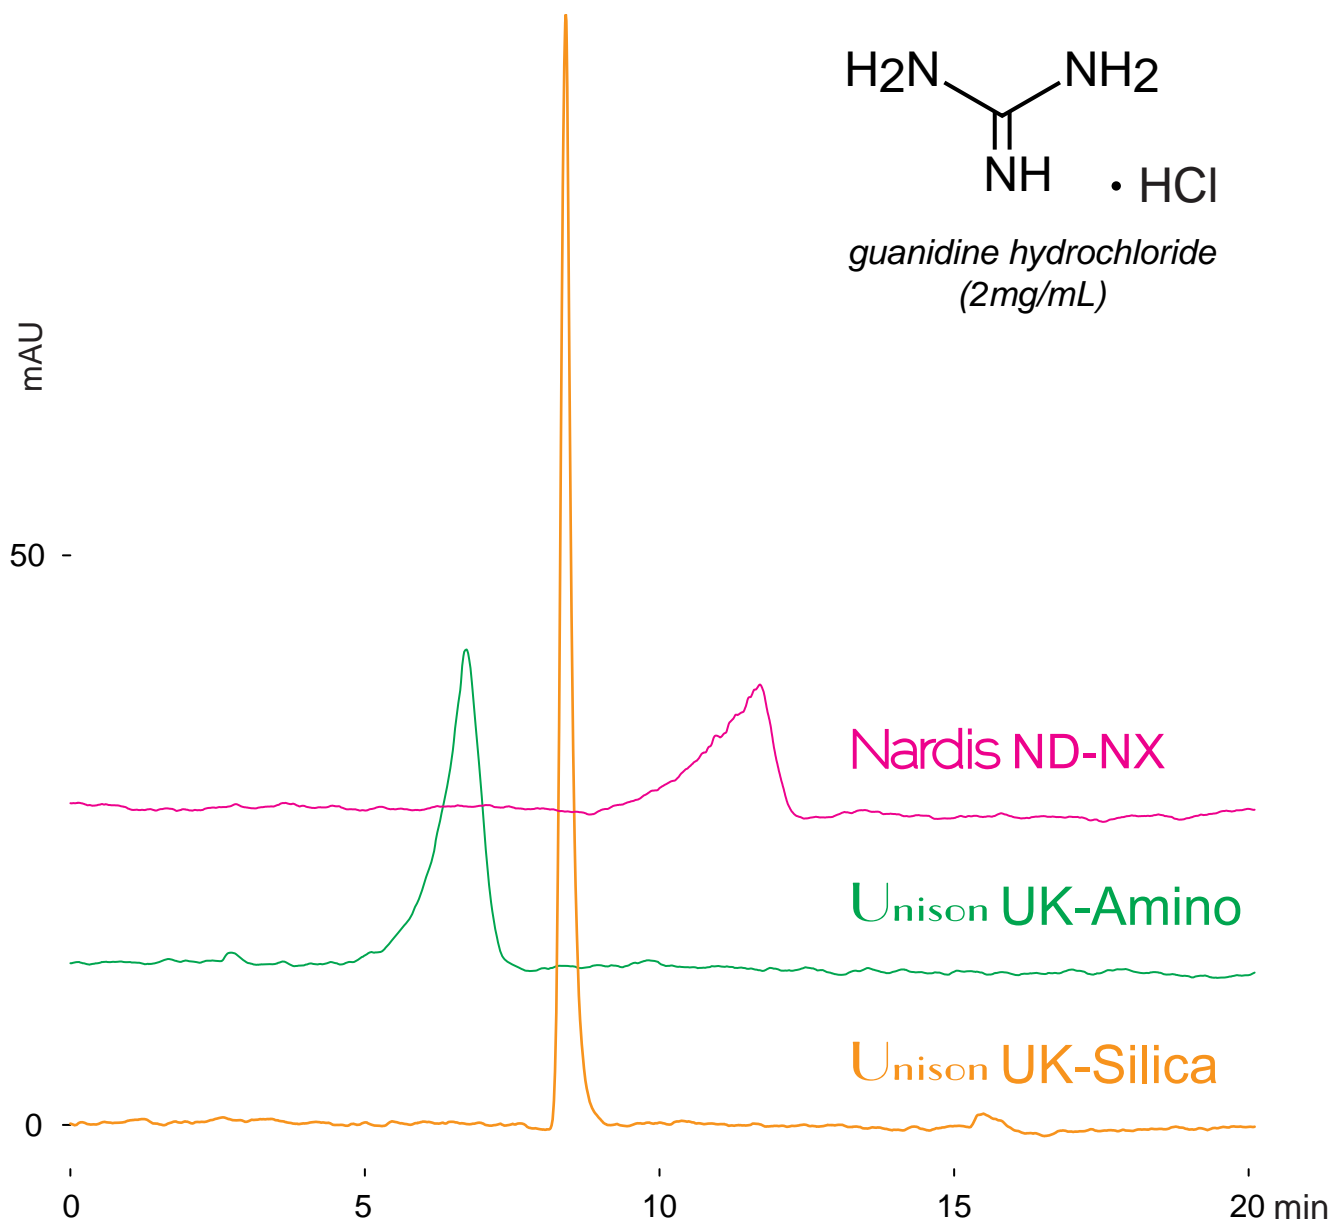

150 x 4.6 mm

A: acetonitrile / acetic acid = 100 / 0.5

B: acetonitrile / water / acetic acid = 50 / 50 / 0.5

0-50%B (0-15min)

1.0mL/min (5-7MPa), 37°C

ELSD (spray chamber 70°C, drift chamber 100°C)

10µL (2mg/mL, water)